

CB-7011/CB-7011D, CB-7018 User's Manual



**MEASUREMENT
COMPUTING™**

Copyright Sept., 2000 All rights are reserved.

Table of Contents

1. Introduction	5
1.1 More Information.....	5
1.2 Pin Assignment.....	6
1.3 Specifications	8
1.4 Block Diagram	11
1.5 Wire Connection.....	12
1.6 Quick Start	14
1.7 Default Setting	14
1.8 Jumper Setting	14
1.9 Calibration.....	15
1.10 Configuration Tables	16
2. Command.....	20
2.1 %AANNTTCCFF	22
2.2 #**	23
2.3 #AA	24
2.4 #AAN	25
2.5 \$AA0	26
2.6 \$AA1	27
2.7 \$AA2	28
2.8 \$AA3	29
2.9 \$AA4	30
2.10 \$AA5VV	31

2.11	\$AA6	32
2.12	\$AA8	33
2.13	\$AA8V	34
2.14	\$AA9(Data)	35
2.15	\$AAB	36
2.16	\$AAF	37
2.17	\$AAM	38
2.18	\$AAZ(Data)	39
2.19	~AAO(Data)	40
2.20	~AAEV	41
2.21	@AADI	42
2.22	@AADO(Data)	44
2.23	@AAEAT	45
2.24	@AAHI(Data)	46
2.25	@AALO(Data)	47
2.26	@AADA	48
2.27	@AACA	49
2.28	@AARH	50
2.29	@AARL	51
2.30	@AARE	52
2.31	@AACE	53
2.32	~**	54
2.33	~AA0	55
2.34	~AA1	56

2.35 ~AA2	57
2.36 ~AA3EVV	58
2.37 ~AA4	59
2.38 ~AA5PPSS	60
3. Application Note.....	61
3.1 INIT* pin Operation	61
3.2 Module Status	61
3.3 Dual Watchdog Operation	62
3.4 Digital Input and Event Counter	62
3.5 Digital Output.....	62
3.6 High/Low Alarm.....	63
3.7 Thermocouple Measurement.....	63

1. Introduction

CB-7000 is a family of network data acquisition and control modules. They provide analog-to-digital, digital-to-analog, digital input/output, timer/counter and other functions. These modules can be remote controlled by a set of commands. The common features of CD-7011/CB-7011D, CB-7018 are as follows:

- 3000VDC isolated analog input
- 24-bits sigma-delta ADC to provide excellent accuracy
- Thermocouples are directly connected with built-in CJC
- Software calibration

The CB-7011 is a single channel analog input module. The CB-7011D is the CB-7011 with a 4½ digit LED display. The CB-7018 is a 8-channel analog input module. The CB-7011P/11PD/18P are enhanced versions of CB-7011/11D/18. The CB-7011P/11PD/18P support two additional thermocouple types and enhance the measurement range of some types.

1.1 More Information

Refer to “**CB-7000 Bus Converter User Manual**” chapter 1 for more information as following:

1.1 CB-7000 Overview


1.2 CB-7000 Related Documentation


1.3 CB-7000 Command Features

1.4 CB-7000 System Network Configuration

1.5 CB-7000 Dimensions

1.2 Pin Assignments

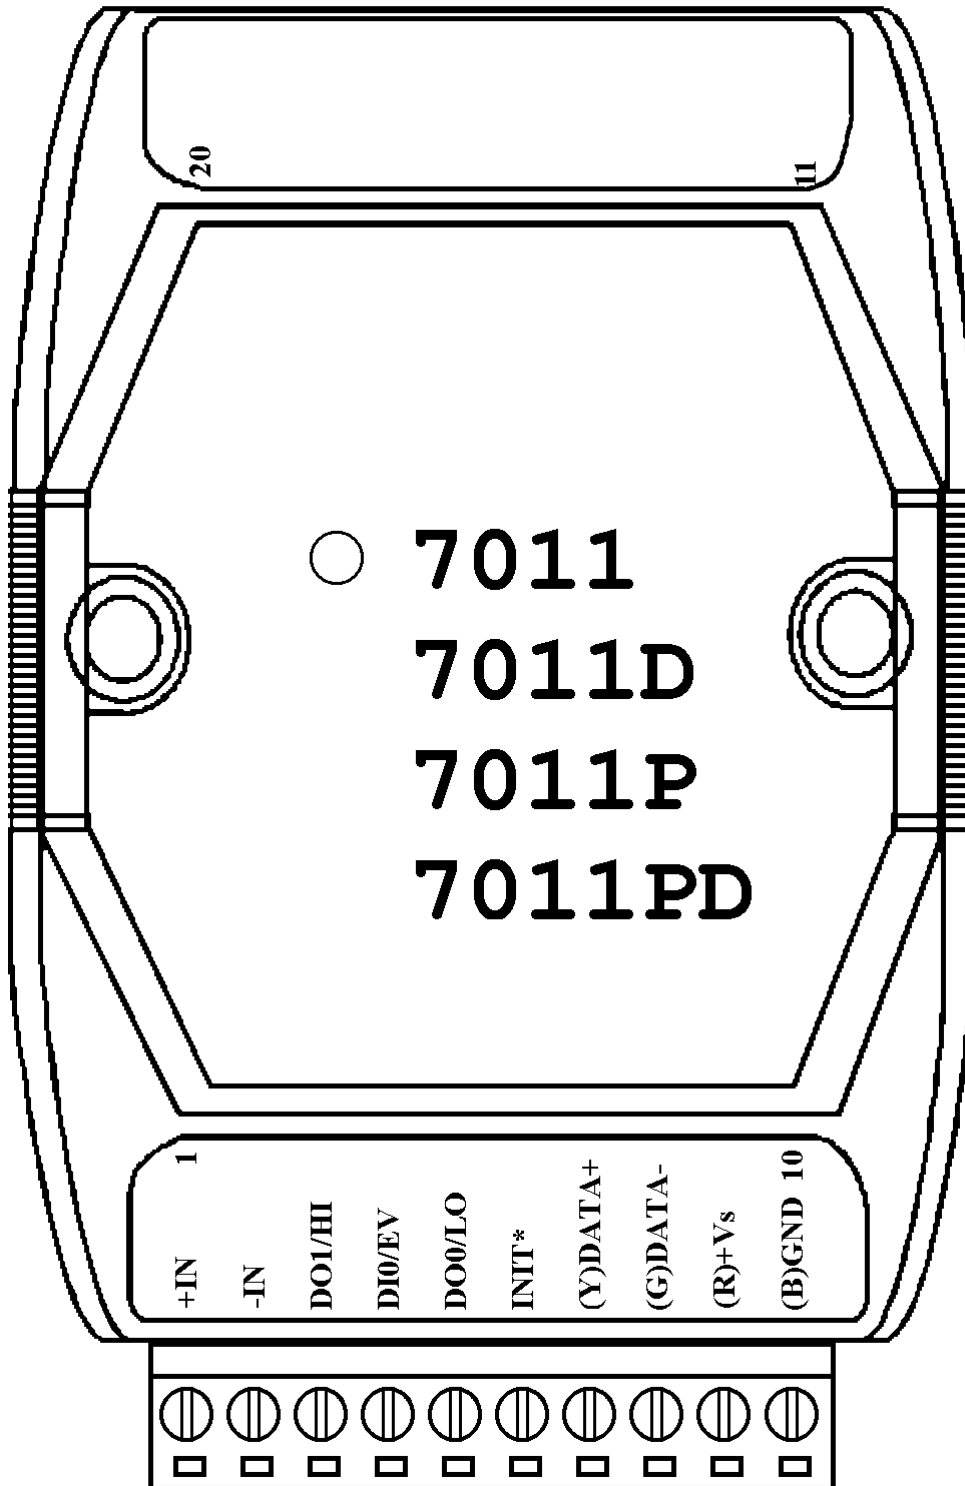

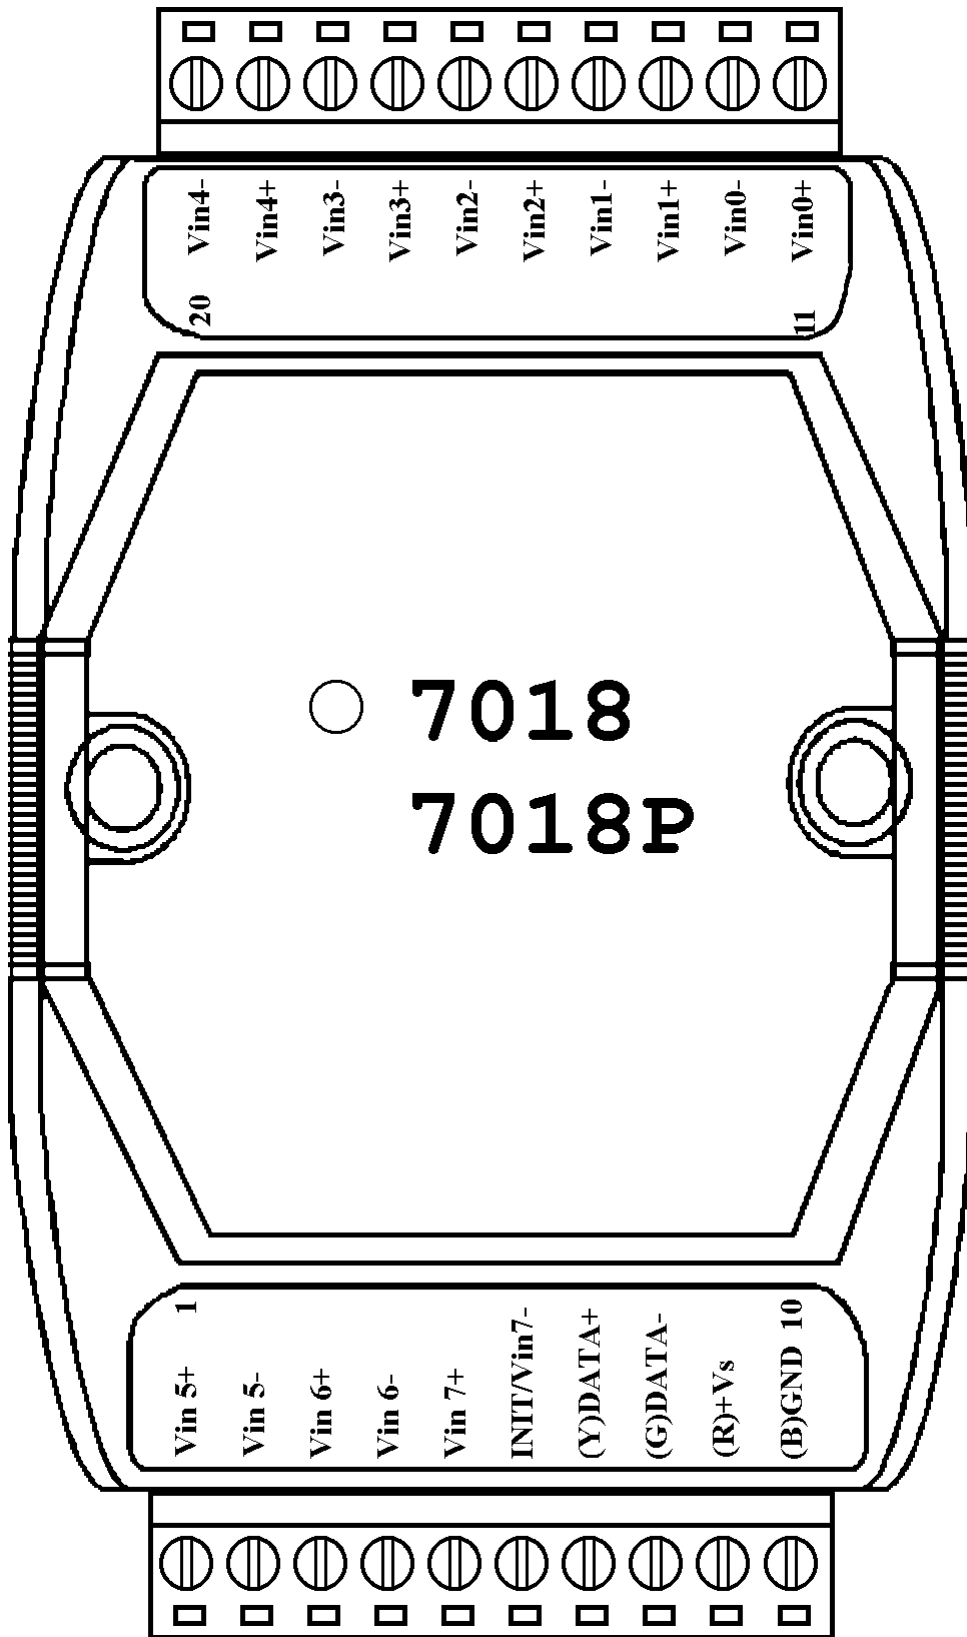

1.3 Specifications

CB-7011/CB-7011D

Analog Input

Input Channel: 1

Input Type:

mV, V, mA (with external
125 ohm resistor)

Thermocouple: Type J, K,
T, E, R, S, B, N, and C

Sampling Rate:

10 Samples/Second

Bandwidth: 5.24 Hz

Accuracy: $\pm 0.05\%$

Zero Drift: $0.5\mu\text{V}/^\circ\text{C}$

Span Drift: 25 ppm/ $^\circ\text{C}$

CMR@50/60Hz: 150dB

NMR@50/60Hz: 100dB

Input Impedance: 20M Ohms

Isolation: 3000VDC

Digital Output

2 channel

Open Collector to 30V

Output Load: sink 30 mA max

Power Dissipation: 300 mW

Digital Input

1 channel

Logic Level 0: +1V max

Logic Level 1: +3.5 to 30V

Event Counter

Max Input Frequency: 50 Hz

Min. Pulse Width: 1 ms

Displayed LED

4½ digits (for CB-7011D)

Power Supply

Input: +10 to +30 VDC

Consumption:

0.9 W for CB-7011

1.5 W for CB-7011D

CB-7011P/CB-7011PD

Analog Input

Input Channel: 1

Input Type:

mV, V, mA(with external
125 ohms resistor)

Thermocouple: Type J, K,
T, E, R, S, B, N, C, L, M

Sampling Rate:

10 Samples/Second

Bandwidth: 5.24 Hz

Accuracy: $\pm 0.05\%$

Zero Drift: $0.5\mu\text{V}/^\circ\text{C}$

Span Drift: $25\text{ppm}/^\circ\text{C}$

CMR@50/60Hz: 150dB

NMR@50/60Hz: 100dB

Input Impedance: 20M Ohms

Isolation: 3000VDC

Digital Output

2 channel

Open Collector to 30V

Output Load: sink 30mA max

Power Dissipation: 300mW

Digital Input

1 channel

Logic Level 0: +1V max

Logic Level 1: +3.5 to 30V

Event Counter

Max Input Frequency: 50 Hz

Min. Pulse Width: 1 ms

Displayed LED

4½ digits (for CB-7011PD)

Power Supply

Input: +10 to +30 VDC

Consumption:

0.9W for CB-7011P

1.5W for CB-7011PD

CB-7018

Analog Input

Input Channel:

8 differential or 6 differential and 2 single-ended.
Jumper select.

Input Type:

mV, V, mA(with external 125 ohms resistor)
Thermocouple: Type J, K, T, E, R, S, B, N, C

Sampling Rate:

10 Samples/Second

Bandwidth: 15.7 Hz

Accuracy: $\pm 0.1\%$

Zero Drift: $0.5\mu\text{V}/^\circ\text{C}$

Span Drift: $25\text{ppm}/^\circ\text{C}$

CMR @ 50/60Hz: 150dB

NMR @ 50/60Hz: 100dB

Input Impedance: 20 MOhms

Overvoltage Protection: $\pm 35\text{V}$

Isolation: 3000VDC

Power Supply

Input: +10 to +30 VDC

Consumption: 1.0W

CB-7018P

Analog Input

Input Channel:

8 differential or 6 differential and 2 single-ended.
Jumper-selected.

Analog Input Type:

mV, V, mA(with external 125 ohms resistor)
Thermocouple: Type J, K, T, E, R, S, B, N, C, L, M

Sampling Rate:

10 Samples/Second

Bandwidth: 15.7 Hz

Accuracy: $\pm 0.1\%$

Zero Drift: $0.5\mu\text{V}/^\circ\text{C}$

Span Drift: $25\text{ppm}/^\circ\text{C}$

CMR @ 50/60Hz: 150dB

NMR @ 50/60Hz: 100dB

Input Impedance: 20 MOhms

Overvoltage Protection: $\pm 35\text{V}$



Isolation: 3000VDC

Power Supply

Input: +10 to +30 VDC

Consumption: 1.0W


1.4 Block Diagram

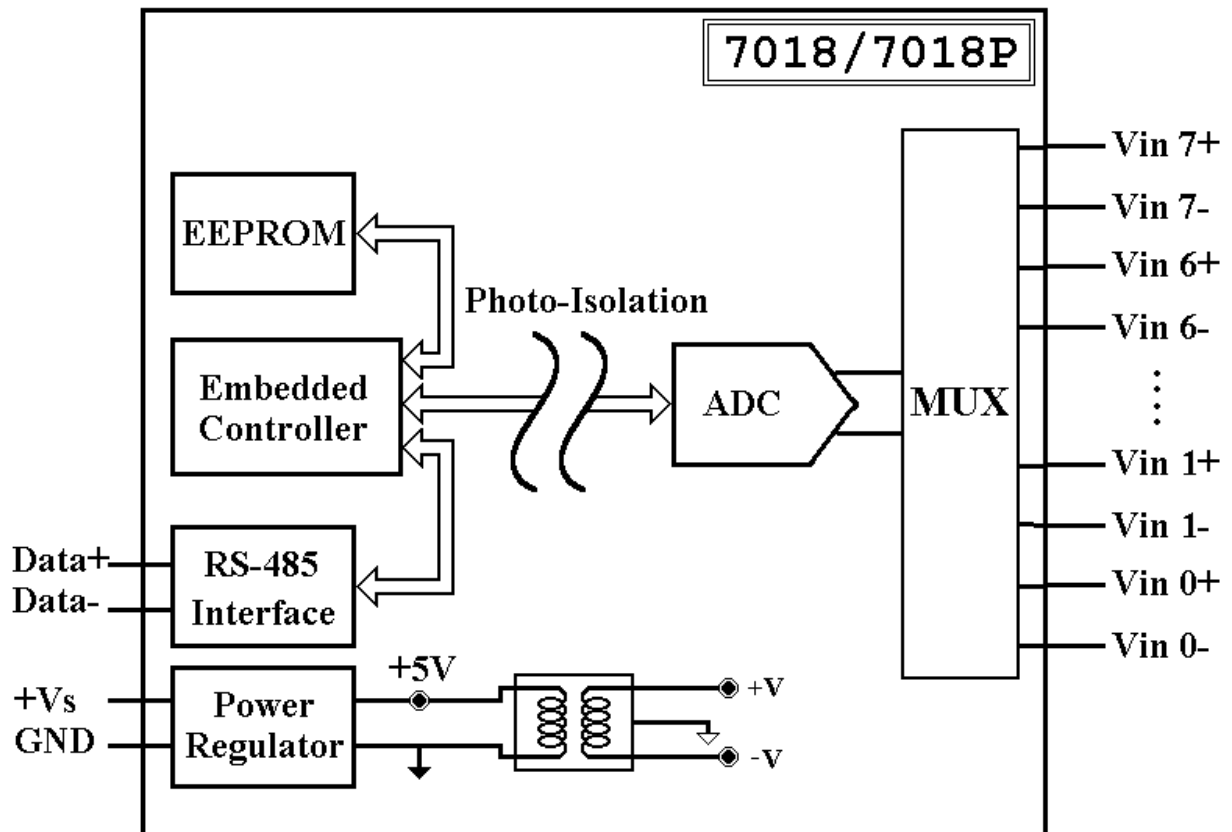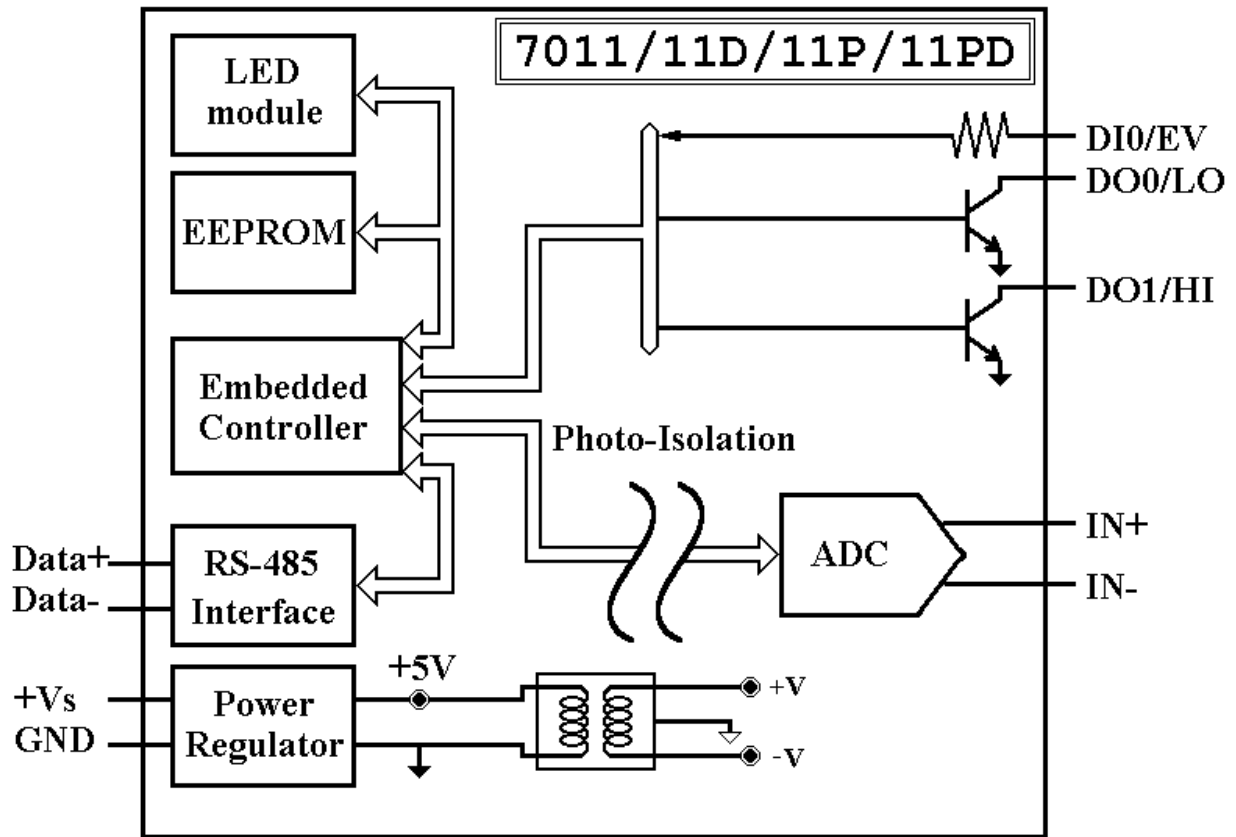

1.5 Wire Connection


CB-7011/11D/11P/11PD

Analog Input Wire Connection

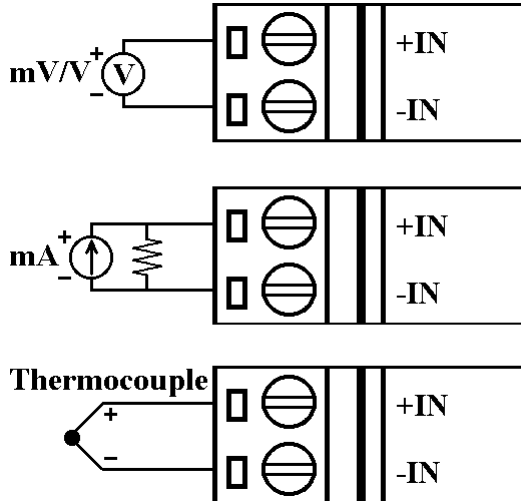


CB-7011/11D/11P/11PD


Digital Output Wire Connection

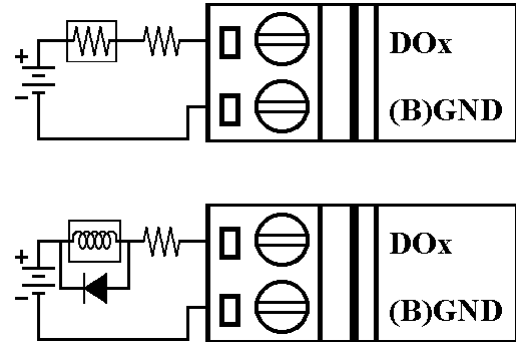

CB-7011/11D/11P/11PD Digital Input Wire Connection

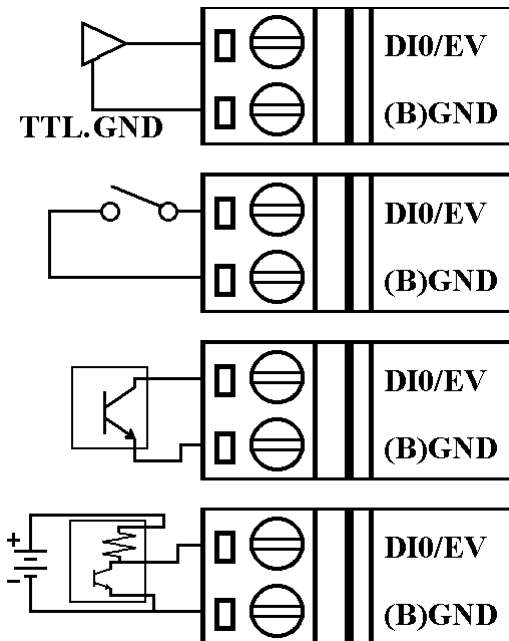



CB-7018/18P Analog Input Channel 0 to 5 Wire Connection

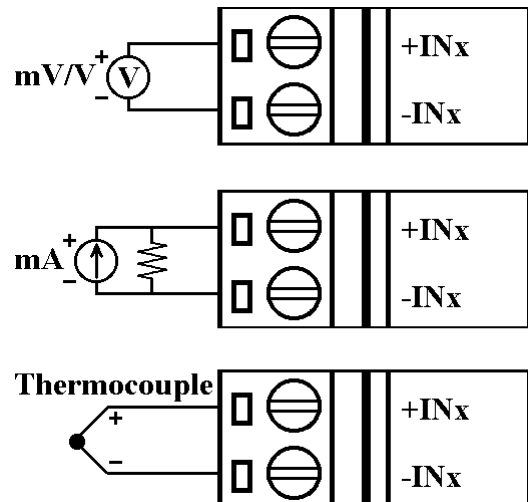

CB-7018/18P Analog Input Channel 6 and 7 Wire Connection, while the jumper JP1 setting is 8 differential mode.

(Remove the cover to gain access to jumper JP1.)

CB-7018/18P Analog Input Channel 6 and 7 Wire Connection, while the jumper JP1 setting is INIT* mode.

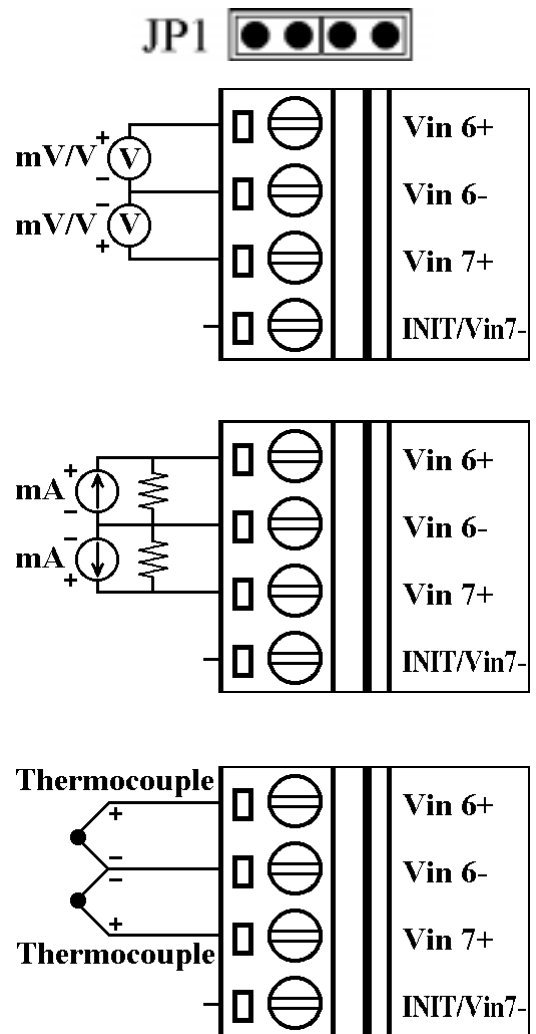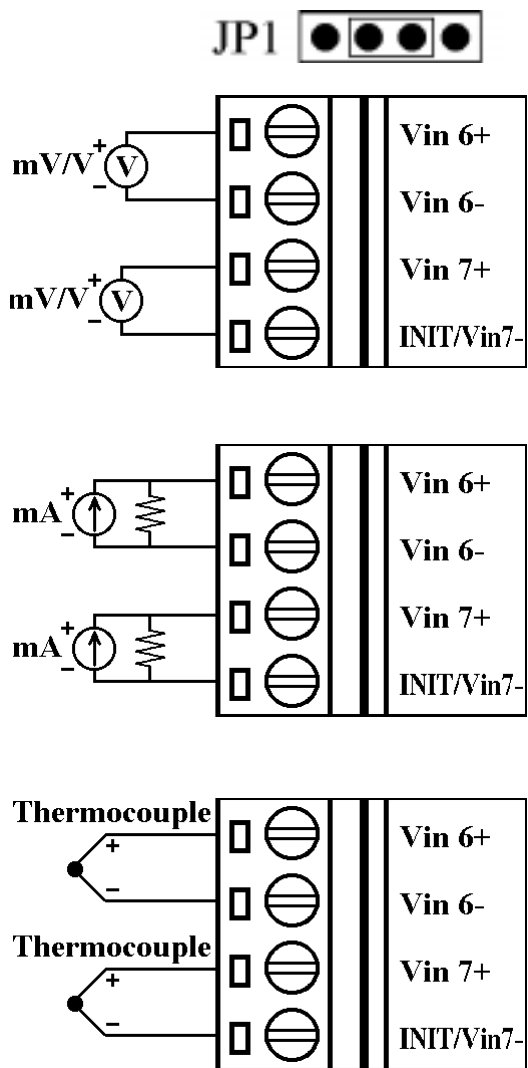

1.6 Quick Start

Refer to “**CB-7000 Bus Converter User Manual**” and “**Getting Start**” for more details.

1.7 Default Setting

Default setting for CB-7011/11D/11P/11PD/18/18P:

- Address: 01
- Analog Input Type: Type 05, -2.5 to +2.5 V
- Baud rate: 9600 bps
- Checksum disable, 60 Hz rejection, engineering unit format
- CB-7018/18P set as INIT* mode; there are six differential and two single-ended analog inputs.

1.8 Jumper Setting

CB-7018/18P: Jumper JP1 for select the pin INIT*/Vin 7-

Select 8 differential mode; the pin INIT*/Vin7- is set to Vin7-



Select INIT* mode; the pin INIT*/Vin7- is set to INIT*



1.9 Calibration

Read Carefully Before Performing Calibration

Calibration Requirement for CB-7011/11D/11P/11PD/18/18P:

Type Code	00	01	02	03	04	05	06
Min. Input	0 mV	0 mV	0 mV	0 mV	0 V	0 V	0 mA
Max Input	+15 mV	+50 mV	+100 mV	+500 mV	+1 V	+2.5 V	+20 mA

Notification:

1. When calibrating a type 06, connect an external shunt resistor, 125 ohms, 0.1% (Ref *Sec. 1.5*).
2. Connect calibration voltage (or current) signal to module's input. For CB-7018/18P, connect to channel 0. (For wire connection reference, *see Sec. 1.5*)
3. Before calibration, warm-up the module for about 30 minutes to improve the accuracy.

Example Calibration Sequence for Type 00:

1. Set Type to 00. Refer to *Sec. 2.1*.
2. Enable Calibration. Refer to *Sec. 2.20*.
3. Apply Zero Calibration Voltage (0 mV)
4. Perform Zero Calibration Command Refer to *Sec. 2.6*.
5. Apply Span Calibration Voltage (15mV)
6. Perform Span Calibration Command Refer to *Sec. 2.5*.
7. Repeat step 1 to step 6 three times.

Calibration sequence for other type is similiar but different in step 1 to set different a type.

1.10 Configuration Tables

Configuration Table of CB-7011/11D/11P/11PD/18/18P:

Baud rate Setting (CC)

Code	03	04	05	06	07	08	09	0A
Baudrate	1200	2400	4800	9600	19200	38400	57600	115200

Analog Input Type Setting (TT)

Type Code	00	01	02	03	04	05	06
Min. Input	-15 mV	-50 mV	-100 mV	-500 mV	-1 V	-2.5 V	-20 mA
Max Input	+15 mV	+50 mV	+100 mV	+500 mV	+1 V	+2.5 V	+20 mA

Type Code	0E	0F	10	11	12	13	14	15	16	17	18
TC Type	J	K	T	E	R	S	B	N	C	L	M
Min Temp	0	-200	-200	-200	0	0	0	-270	0	-200	-200
Max Temp	750	1250	350	900	1450	1450	1700	1300	2320	800	100
The temperatures shown are in degrees Celsius.											

T.C. Type L and M for CB-7011P/11PD/18P only.

Data Format Setting (FF)

7	6	5	4	3	2	1	0
*1	*2	0	0	0	0	*3	

*1: Filter Select: 0 = 60 Hz rejection

1 = 50 Hz rejection

*2: Checksum Bit: 0=Disable, 1=Enable

*3: 00 = Engineering Unit Format

01 = Percent Format

10 = 2's Complement HEX Format

Analog Input Type and Data Format Table

Type Code	Input Range	Data Format	+F.S.	Zero	-F.S.
00	-15 to +15 mV	Engineer Unit	+15.000	+00.000	-15.000
		% of FSR	+100.00	+000.00	-100.00
		2's complement HEX	7FFF	0000	8000
01	-50 to +50 mV	Engineer Unit	+50.000	+00.000	-50.000
		% of FSR	+100.00	+000.00	-100.00
		2's complement HEX	7FFF	0000	8000
02	-100 to +100 mV	Engineer Unit	+100.00	+000.00	-100.00
		% of FSR	+100.00	+000.00	-100.00
		2's complement HEX	7FFF	0000	8000
03	-500 to +500 mV	Engineer Unit	+500.00	+000.00	-500.00
		% of FSR	+100.00	+000.00	-100.00
		2's complement HEX	7FFF	0000	8000
04	-1 to +1 V	Engineer Unit	+1.0000	+0.0000	-1.0000
		% of FSR	+100.00	+000.00	-100.00
		2's complement HEX	7FFF	0000	8000
05	-2.5 to +2.5 V	Engineer Unit	+2.5000	+0.0000	-2.5000
		% of FSR	+100.00	+000.00	-100.00
		2's complement HEX	7FFF	0000	8000
06	-20 to +20 mA	Engineer Unit	+20.000	+00.000	-20.000
		% of FSR	+100.00	+000.00	-100.00
		2's complement HEX	7FFF	0000	8000

Type Code	Input Range	Data Format	+F.S.	Zero	-F.S.
0E	J Type -210 to 760 degree Celsius	Engineer Unit	+760.00	+00.000	-210.00
		% of FSR	+100.00	+000.00	-027.63
		2's complement HEX	7FFF	0000	DCA2
0F	K Type -270 to 1372 degree Celsius	Engineer Unit	+1372.0	+00.000	-0270.0
		% of FSR	+100.00	+000.00	-019.68
		2's complement HEX	7FFF	0000	E6D0
10	T Type -270 to 400 degree Celsius	Engineer Unit	+400.00	+000.00	-270.00
		% of FSR	+100.00	+000.00	-067.50
		2's complement HEX	7FFF	0000	A99A
11	E Type -270 to 1000 degree Celsius	Engineer Unit	+1000.0	+000.00	-0270.0
		% of FSR	+100.00	+000.00	-027.00
		2's complement HEX	7FFF	0000	DD71
12	R Type 0 to 1768 degree Celsius	Engineer Unit	+1768.0	+0000.0	+0000.0
		% of FSR	+100.00	+0000.0	+0000.0
		2's complement HEX	7FFF	0000	0000
13	S Type 0 to 1768 degree Celsius	Engineer Unit	+1786.0	+0.0000	+0000.0
		% of FSR	+100.00	+000.00	+0000.0
		2's complement HEX	7FFF	0000	0000
14	B Type 0 to 1820 degree Celsius	Engineer Unit	+1820.0	+00.000	+0000.0
		% of FSR	+100.00	+000.00	+0000.0
		2's complement HEX	7FFF	0000	0000
15	N Type -270 to 1300 degree Celsius	Engineer Unit	+1300.0	+00.000	-0270.0
		% of FSR	+100.00	+000.00	-20.77
		2's complement HEX	7FFF	0000	E56B

Type Code	Input Range	Data Format	+F.S.	Zero	-F.S.
16	C Type 0 to 2320 degree Celsius	Engineer Unit	+2320.0	+00.000	+00.000
		% of FSR	+100.00	+000.00	+000.00
		2's complement HEX	7FFF	0000	0000
17* ¹	L Type -200 to 800 degree Celsius	Engineer Unit	+800.00	+00.000	-200.00
		% of FSR	+100.00	+000.00	-025.00
		2's complement HEX	7FFF	0000	E000
18* ¹	M Type -200 to 100 degree Celsius	Engineer Unit	+100.00	+000.00	-200.00
		% of FSR	+050.00	+000.00	-100.00
		2's complement HEX	4000	0000	8000
* ¹ : Only available for 7011P, 7011PD and 7018P					

2. Command

Command Format: **(Leading)(Address)(Command)[CHK](cr)**

Response Format: **(Leading)(Address)(Data)[CHK](cr)**

[CHK] 2-character checksum

(cr) end-of-command character, character return(0x0D)

General Command Sets			
Command	Response	Description	Section
%AANNTTCCFF	!AA	Set Module Configuration	<i>Sec.2.1</i>
#**	No Response	Synchronized Sampling	<i>Sec.2.2</i>
#AA	>(Data)	Read Analog Input	<i>Sec.2.3</i>
#AAN	>(Data)	Read Analog Input from channel N	<i>Sec.2.4</i>
\$AA0	!AA	Perform Span Calibration	<i>Sec.2.5</i>
\$AA1	!AA	Perform Zero Calibration	<i>Sec.2.6</i>
\$AA2	!AATTCCFF	Read Configuration	<i>Sec.2.7</i>
\$AA3	>(Data)	Read CJC Temperature	<i>Sec.2.8</i>
\$AA4	>AAS(Data)	Read Synchronized Data	<i>Sec.2.9</i>
\$AA5VV	!AA	Set Channel Enable	<i>Sec.2.10</i>
\$AA6	!AAVV	Read Channel Status	<i>Sec.2.11</i>
\$AA8	!AAV	Read LED Configuration	<i>Sec.2.12</i>
\$AA8V	!AA	Set LED Configuration	<i>Sec.2.13</i>
\$AA9(Data)	!AA	Set CJC Offset Value	<i>Sec.2.14</i>
\$AAB	!AAS	T.C. Open Detection	<i>Sec.2.15</i>
\$AAF	!AA(Data)	Read Firmware Version	<i>Sec.2.16</i>
\$AAM	!AA(Data)	Read Module Name	<i>Sec.2.17</i>
\$AAZ(Data)	!AA	Send LED Data	<i>Sec.2.18</i>

General Command Sets (Continued)			
~AAO(Data)	!AA	Set Module Name	<i>Sec.2.19</i>
~AAEV	!AA	Enable/Disable Calibration	<i>Sec.2.20</i>
Digital Input/Output, Alarm and Event Counter Command Sets			
@AADI	!AASOOII	Read Digital I/O and Alarm Status	<i>Sec.2.21</i>
@AADO(Data)	!AA	Set Digital Output	<i>Sec.2.22</i>
@AAEAT	!AA	Enable Alarm	<i>Sec.2.23</i>
@AAHI(Data)	!AA	Set High Alarm	<i>Sec.2.24</i>
@AALO(Data)	!AA	Set Low Alarm	<i>Sec.2.25</i>
@AADA	!AA	Disable Alarm	<i>Sec.2.26</i>
@AACA	!AA	Clear Latch Alarm	<i>Sec.2.27</i>
@AARH	!AA(Data)	Read High Alarm	<i>Sec.2.28</i>
@AARL	!AA(Data)	Read Low Alarm	<i>Sec.2.29</i>
@AARE	!AA(Data)	Read Event Counter	<i>Sec.2.30</i>
@AACE	!AA	Clear Event Counter	<i>Sec.2.31</i>
Host Watchdog Command Sets			
~**	No Response	Host OK	<i>Sec.2.32</i>
~AA0	!AASS	Read Module Status	<i>Sec.2.33</i>
~AA1	!AA	Reset Module Status	<i>Sec.2.34</i>
~AA2	!AAVV	Read Host Watchdog Timeout Value	<i>Sec.2.35</i>
~AA3EVV	!AA	Set Host Watchdog Timeout Value	<i>Sec.2.36</i>
~AA4	!AAPPSS	Read PowerOn Value and Safe Value	<i>Sec.2.37</i>
~AA5PPSS	!AA	Set PowerOn Value and Safe Value	<i>Sec.2.38</i>

2.1 %AANNTCCFF

Description: Set module Configuration

Syntax: %AANNTCCFF[CHK](cr)

% a delimiter character

AA address of setting module (00 to FF)

NN new address for setting module (00 to FF)

TT new type for setting module (Ref. *Sec. 1.10*)

CC new baudrate for setting module (Ref. *Sec. 1.10*)

FF new data format for setting module (Ref. *Sec. 1.10*)

When changing the baud rate or checksum, it is necessary to short the INIT* pin to ground.

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

A syntax error or communication error may yield no response.

! delimiter for valid command

? delimiter for invalid command. If you change baud rate or checksum setting without shorting INIT* to ground, the module will return invalid command.

AA address of response module (00 to FF)

Example:

Command: %0102050600 Receive: !02

Change address from 01 to 02, return success.

Related Command:

\$AA2 (*Sec. 2.7*)

Related Topics:

Configuration Tables (*Sec. 1.10*), INIT* pin Operation (*Sec. 3.1*)

2.2 #**

Description: Synchronized Sampling

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: #**[CHK](cr)

a delimiter character

** synchronized sampling command

Response: No response

Example:

Command: \$014 Receive: ?01

Read synchronized sampling data, returns no valid data .

Command: #** No response

Send synchronized sampling command.

Command: \$014 Receive: >011+025.123

First read, get status=1, first read.

Command: \$014 Receive: >010+025.123

Second read, get status=0, read verified.

Related Command:

\$AA4 (*Sec. 2.9*)

2.4 #AAN

Description: Read Analog Input from channel N

Note: The command is for CB-7018/18P only.

Syntax: #AAN[CHK](cr)

- # delimiter character
AA address of reading module (00 to FF)
N channel to read, from 0 to 7

Response: Valid Command: >(Data)[CHK](cr)

 Invalid Command: ?AA[CHK](cr)

 Syntax error or communication error may get no response.

> delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

(Data) analog input value, reference *Sec. 1.10* for its format

Example:

Command: #032 Receive: >+02.513

 Read address 03 channel 2, get data success.

Command: #029 Receive: ?02

 Read address 02 channel 9, return error channel number.

Related Command:

%AANNTTCCFF (*Sec. 2.1*), \$AA2 (*Sec 2.7*)

Related Topics:

Configuration Tables (*Sec. 1.10*)

2.5 \$AA0

Description: Perform Span Calibration

Syntax: \$AA0[CHK](cr)

\$ delimiter character

AA address of setting module (00 to FF)

0 command for performing span calibration

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command or the calibration is not enabled

AA address of response module(00 to FF)

Example:

Command: \$010 Receive: !01

Perform address 01 span calibration, return success.

Command: \$020 Receive: ?02

Perform address 02 span calibration, return the calibration is not enabled before perform calibration command.

Related Command:

\$AA1 (*Sec. 2.6*), ~AAEV (*Sec. 2.20*)

Related Topics:

Calibration (*Sec. 1.9*)

2.6 \$AA1

Description: Perform Zero Calibration

Syntax: \$AA1[CHK](cr)

\$ delimiter character

AA address of setting module (00 to FF)

1 command for performing zero calibration

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command or the calibration is not enabled

AA address of response module(00 to FF)

Example:

Command: \$011 Receive: !01

Perform address 01 zero calibration, return success.

Command: \$021 Receive: ?02

Perform address 02 zero calibration, return the calibration is not enabled before perform calibration command.

Related Command:

\$AA0 (*Sec. 2.5*), ~AAEV (*Sec. 2.20*)

Related Topics:

Calibration (*Sec. 1.9*)

2.7 \$AA2

Description: Read Configuration

Syntax: \$AA2[CHK](cr)

\$ delimiter character

AA address of reading module (00 to FF)

2 command for reading configuration

Response: Valid Command:

!AATTCCFF[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

TT type code of module (reference *Sec. 1.10*)

CC baudrate code of module (reference *Sec. 1.10*)

FF data format of module (reference *Sec. 1.10*)

Example:

Command: \$012 Receive: !01050600

 Read address 01 configuration, return success.

Command: \$022 Receive: !02030602

 Read address 02 configuration, return success.

Related Command:

%AANNTTCCFF (*Sec. 2.1*)

Related Topics:

Config. Tables (*Sec. 1.10*), INIT* pin Operation (*Sec. 3.1*)

2.8 \$AA3

Description: Read CJC Temperature

Syntax: \$AA3[CHK](cr)

\$ delimiter character

AA address of reading module (00 to FF)

3 command for reading CJC temperature

Response: Valid Command: >(Data)[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

> delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

(Data) CJC temperature in degrees Celsius.

Example:

Command: \$033 Receive: >+0025.4

Read address 03 CJC temperature, return 25.4°C.

Related Command:

\$AA9(Data) (*Sec. 2.14*)

2.9 \$AA4

Description: Read Synchronized Data

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: \$AA4[CHK](cr)

\$ delimiter character

AA address of reading module (00 to FF)

4 command for reading synchronized data

Response: Valid Command: >AAS(Data)[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command or the module does not receive command #** before the command \$AA4.

AA address of response module(00 to FF)

S status of synchronized data, 1 = first time read, 0 = has been read

(Data) synchronized data, format reference *Sec. 1.10*

Example:

See example of *Sec. 2.2 #***

Related Command:

*Sec. 2.2 #***

2.10 \$AA5VV

Description: Set Channel Enable

Note: The command is for CB-7018/18P only.

Syntax: \$AA5VV[CHK](cr)

\$ delimiter character

AA address of setting module (00 to FF)

5 command for setting channel enable

VV channel enable/disable, 00 is all disabled, and FF is all enabled.

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: \$0155A Receive: !01

Set address 01 enable channel 1,3,4,6 and disable channel 0,2,5,7, return success.

Command: \$016 Receive: !015A

Read address 01 channel status, return channel 1,3,4,6 enable and channel 0,2,5,7 disable.

Related Command:

\$AA6 (*Sec. 2.11*)

2.11 \$AA6

Description: Read Channel Status

Note: The command is for CB-7018/18P only.

Syntax: \$AA6[CHK](cr)

\$ delimiter character

AA address of reading module (00 to FF)

6 command for reading channel status

Response: Valid Command: !AAVV[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

VV channel enable/disable, 00 is all disabled, and FF is all enabled.

Example:

Command: \$015A5 Receive: !01

Set address 01, enable channel 0,2,5,7 and disable channel 1,3,4,6 , return success.

Command: \$016 Receive: !01A5

Read address 01 channel status, return channel 0,2,5,7 enable and channel 1,3,4,6 disable.

Related Command:

\$AA5VV (*Sec. 2.10*)

2.12 \$AA8

Description: Read LED Configuration

Note: The command is for CB-7011D/11PD only.

Syntax: \$AA8[CHK](cr)

\$ delimiter character

AA address of reading module (00 to FF)

8 command for setting LED configuration

Response: Valid Command: !AAV[CHK](cr)

 Invalid Command: ?AA[CHK](cr)

 Syntax error or communication error may get no re-
 sponse.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

V LED configuration

 1=module control, 2=host control

Example:

Command: \$018 Receive: !011

 Read address 01 LED configuration, return module control.

Command: \$028 Receive: !012

 Read address 02 LED configuration, return host control.

Related Command:

\$AA8V (*Sec. 2.13*), \$AAZ(Data) (*Sec. 2.18*)

2.13 \$AA8V

Description: Set LED Configuration

Note: The command is for CB-7011D/11PD only.

Syntax: \$AA8V[CHK](cr)

\$ delimiter character

AA address of setting module (00 to FF)

8 command for setting LED configuration

V 1=Set LED to module, 2=Set LED to host

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: \$0182 Receive: !01

Set address 01 LED to host control, return success.

Command: \$0281 Receive: !02

Set address 02 LED to module control, return success.

Related Command:

\$AA8 (*Sec. 2.12*), \$AAZ(Data) (*Sec. 2.18*)

2.14 \$AA9(Data)

Description: Set CJC Offset Value

Syntax: \$AA9(Data)[CHK](cr)

\$ delimiter character

AA address of setting module (00 to FF)

9 command for setting CJC offset value

(Data) CJC offset value comprises a sign and 4 hexadecimal digits, from -1000 to +1000, each count is 0.01°C.

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module (00 to FF)

Example:

Command: \$019+0010 Receive: !01

Set address 01 CJC offset increase 16 counts (+0.16°C), return success.

Related Command:

\$AA3 (*Sec. 2.8*)

2.15 \$AAB

Description: Thermocouple Open Detection

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: \$AAB[CHK](cr)

\$ delimiter character

AA address of reading module (00 to FF)

B command for reading thermocouple open status

Response: Valid Command: !AAS[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

S 0=close-loop detection

1=open-circuit detection, need to check the thermocouple

Example:

Command: \$01B

Receive: !010

Read address 01, thermocouple open status, return the thermocouple is close-loop.

2.16 \$AAF

Description: Read Firmware Version

Syntax: \$AAF[CHK](cr)

\$ delimiter character

AA address of reading module (00 to FF)

F command for reading firmware version

Response: Valid Command: !AA(Data)[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

(Data) firmware version of module

Example:

Command: \$01F Receive: !01A2.0

Read address 01 firmware version, return version A2.0.

Command: \$02F Receive: !01B1.1

Read address 02 firmware version, return version B1.1.

2.17 \$AAM

Description: Read Module Name

Syntax: \$AAM[CHK](cr)

\$ delimiter character

AA address of reading module (00 to FF)

M command for reading module name

Response: Valid Command: !AA(Data)[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

(Data) Name of module

Example:

Command: \$01M Receive: !017018

Read address 01 module name, return name 7018.

Command: \$03M Receive: !037011D

Read address 03 module name, return name 7011D.

Related Command:

~AAO(Data) (*Sec. 2.19*)

2.18 \$AAZ(Data)

Description: Set LED Data

Note: The command is for CB-7011D/11PD only.

Syntax: \$AAZ(Data)[CHK](cr)

\$ delimiter character

AA address of setting module (00 to FF)

Z command for setting LED data

(Data) data for show on the LED, from -19999. to +19999. The data need sign, 5 digits and decimal point.

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command or LED not set to host control

AA address of response module (00 to FF)

Example:

Command: \$01Z+123.45 Receive: !01

Send address 01 LED data +123.45, return success.

Command: \$02Z+512.34 Receive: ?02

Send address 02 LED data +512.34, return the LED is not setting in the host mode.

Related Command:

\$AA8 (Sec. 2.12), \$AA8V (Sec. 2.13)

2.19 ~AAO(Data)

Description: Set Module Name

Syntax: ~AAO(Data)[CHK](cr)

~ delimiter character
AA address of setting module (00 to FF)
O command for setting module name
(Data) new name for module, max 6 characters

Response: Valid Command: !AA[CHK](cr)

 Invalid Command: ?AA[CHK](cr)

 Syntax error or communication error may get no
 response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: ~01O7018 Receive: !01

 Set address 01 module name to 7018, return success.

Command: \$01M Receive: !017018

 Read address 01 module name, return 7018.

Related Command:

\$AAM (*Sec. 2.17*)

2.20 ~AAEV

Description: Enable/Disable Calibration

Syntax: ~AAEV[CHK](cr)

~ delimiter character

AA address of setting module (00 to FF)

E command for enable/disable calibration

V 1=enable calibration, 0=disable calibration

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: \$010 Receive: ?01

Perform address 01 span calibration, return it is not ready for calibration.

Command: ~01E1 Receive: !01

Set address 01 to enable calibration, return success.

Command: \$010 Receive: !01

Perform address 01 span calibration, return success.

Related Command:

\$AA0 (*Sec. 2.5*), \$AA1 (*Sec. 2.6*)

Related Topic:

Calibration (*Sec. 1.9*)

2.21 @AADI

Description: Read Digital I/O and Alarm Status

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: @AADI[CHK](cr)

@ delimiter character

AA address of reading module (00 to FF)

DI command for reading digital I/O and alarm status

Response: Valid Command: !AASOOII[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

S alarm enable status, 0=alarm disable, 1=momentary alarm enabled, 2=latch alarm enabled.

OO digital output status, 00=DO0 off, DO1 off, 01=DO0 on, DO1 off, 02=DO0 off, DO1 on, 03=OD0 on, DO1 on.

II digital input status, 00=input low level, 01=input high level.

Example:

Command: @01DI Receive: !0100001

Read address 01 digital I/O status, return alarm disable, digital outputs all off, and digital input high level.

Command: @02DI Receive: !0210100

Read address 02 digital I/O status, return momentary alarm

enable, high alarm is clear, low alarm is set, and digital input is high.

Related Command:

@AADO(Data) (*Sec. 2.22*), @AAEAT (*Set. 2.23*), @AADA (*Sec. 2.26*)

Related Topic:

Digital Input and Event Counter (*Sec. 3.4*), Digital Output (*Sec. 3.5*), High/Low Alarm (*Sec. 3.6*)

2.22 @AADO(Data)

Description: Set Digital Output

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: @AADI[CHK](cr)

@ delimiter character

AA address of setting module (00 to FF)

DO command for setting digital output

(Data) output value, 00=DO0 off, DO1 off, 01=DO0 on, DO1 off, 02=DO0 off, DO1 on, 03=DO0 on, DO1 on

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command. When the alarm is enabled, the command will return invalid.

AA address of response module(00 to FF)

Example:

Command: @01DO00 Receive: !01

Set address 01 digital output 00, return success.

Related Command:

@AADI (Sec. 2.21), @AAEAT (Set. 2.23), @AADA (Sec. 2.26)

Related Topic:

Sec. 3.5 Digital Output

2.23 @AAEAT

Description: Enable Alarm

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: @AAEAT[CHK](cr)

@ delimiter character
AA address of setting module (00 to FF)
EA command for enable alarm.
T alarm type, M=momentary alarm, L=latch alarm.

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: @01EAM Receive: ?01

Set address 01 momentary alarm, return success.

Related Command:

@AADA (*Sec. 2.26*), @AACA (*Sec. 2.27*) **Related Topic:**

High/Low Alarm (*Sec. 3.6*)

2.24 @AAHI(Data)

Description: Set High Alarm

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: @AAHI[CHK](cr)

@ delimiter character

AA address of setting module (00 to FF)

HI command for setting high alarm value

(Data) high alarm values, data format is in engineer unit format.

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: @01HI+2.5000 Receive: !01

Set address 01 high alarm +2.5000, return success.

Related Command:

@AAEAT (Sec. 2.23), @AARH (Sec. 2.28)

Related Topic:

High/Low Alarm (Sec. 3.6)

2.25 @AALO(Data)

Description: Set Low Alarm

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: @AADI[CHK](cr)

@ delimiter character

AA address of setting module (00 to FF)

LO command for setting high alarm value

(Data) high alarm values, data format is in engineer unit format.

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: @01LO-2.5000 Receive: !01

Set address 01 low alarm -2.5000, return success.

Related Command:

@AAEAT (Sec. 2.23), @AARL (Sec. 2.29)

Related Topic:

High/Low Alarm (Sec. 3.6)

2.26 @AADA

Description: Disable Alarm

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: @AADA[CHK](cr)

@ delimiter character

AA address of setting module (00 to FF)

DA command for disable alarm

Response Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: @01DA Receive: !01

Disable address 01 alarm, return success.

Related Command:

Sec. 2.23 @AAEAT

Related Topic:

Sec. 3.6 High/Low Alarm

2.27 @AACCA

Description: Clear Latch Alarm

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: @AACCA[CHK](cr)

@ delimiter character

AA address of setting module (00 to FF)

CA command for clear latch alarm

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: @01DI Receive: !0120101

Read address 01 digital input, return latch alarm mode, low alarm is set.

Command: @01CA Receive: !01

Clear address 01 latch alarm, return success.

Command: @01DI Receive: !0120001

Read address 01 digital input, return latch alarm mode, both alarms are clear.

Related Command:

Sec. 2.21 @AADI, Sec. 2.23 @AAEAT, Sec. 2.26 @AADA

Related Topic:

Sec. 3.6 High/Low Alarm

2.28 @AARH

Description: Read High Alarm

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: @AARH[CHK](cr)

@ delimiter character

AA address of reading module (00 to FF)

RH command for reading high alarm

Response: Valid Command: !AA(Data)[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command.

? delimiter for invalid command.

AA address of response module(00 to FF)

(Data) high alarm value in engineer unit format.

Example:

Command: @01RH Receive: !01+2.5000

Read address 01 high alarm, return +2.5000.

Related Command:

Sec. 2.24 @AAHI(Data)

Related Topic:

Sec. 3.6 High/Low Alarm

2.29 @AARL

Description: Read Low Alarm

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: @AARH[CHK](cr)

@ delimiter character

AA address of reading module (00 to FF)

RL command for reading low alarm

Response: Valid Command: !AA(Data)[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command.

? delimiter for invalid command.

AA address of response module(00 to FF)

(Data) low alarm value in engineer unit format.

Example:

Command: @01RL Receive: !01-2.5000

Read address 01 low alarm, return -2.5000.

Related Command:

Sec. 2.25 @AALO(Data)

Related Topic:

Sec. 3.6 High/Low Alarm

2.30 @AARE

Description: Read Event Counter

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: @AARE[CHK](cr)

@ delimiter character

AA address of reading module (00 to FF)

RE command for reading event counter

Response: Valid Command: !AA(Data)[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

(Data) event counter value, from 00000 to 65535.

Example:

Command: @01RE Receive: !0101234

Read address 01 event counter, return 1234.

Related Command:

Sec. 2.31 @AACE

Related Topic:

Sec. 3.4 Digital Input and Event Counter

2.31 @AAACE

Description: Clear Event Counter

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: @AAACE[CHK](cr)

@ delimiter character

AA address of setting module (00 to FF)

CE command for clear event counter

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: @01RE Receive: !0101234

Read address 01 event counter, return 1234.

Command: @01CE Receive: !01

Clear address 01 event counter, return success.

Command: @01RE Receive: !0100000

Read address 01 event counter, return 0.

Related Command:

Sec. 2.30 @AARE

Related Topic:

Sec. 3.4 Digital Input and Event Counter

2.33 ~AA0

Description: Read Module Status

Syntax: ~AA0[CHK](cr)

~ delimiter character
AA address of reading module (00 to FF)
0 command for reading module status

Response: Valid Command: !AASS[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

SS Module Status. The status will store into EEPROM and only may reset by the command ~AA1.

7	6	5	4	3	2	1	0
*1	Reserved				*2	Reserved	

*1: Host watchdog status, 0=Disable, 1=Enable

*2: Host watchdog timeout flag, 0=Clear, 1=Set

Example:

Command: ~010

Receive: !0104

Read address 02 module status, return 04, host watchdog timeout flag is set.

Related Command:

Sec. 2.34 ~AA1

Related Topic:

Sec. 3.2 Module Status, Sec. 3.3 Dual Watchdog Operation

2.34 ~AA1

Description: Reset Module Status

Syntax: ~AA1[CHK](cr)

~ delimiter character
AA address of setting module (00 to FF)
1 command for reset module status

Response: Valid Command: !AA[CHK](cr)
Invalid Command: ?AA[CHK](cr)
Syntax error or communication error may get no response.

! delimiter for valid command
? delimiter for invalid command
AA address of response module(00 to FF)

Example:

Command: ~010 Receive: !0104
Read address 01 module status, return 04, host watchdog timeout flag is set.

Command: ~011 Receive: !01
Reset address 01 module status, return success.

Command: ~010 Receive: !0100
Read address 01 module status, return 00, Module Status is clear.

Related Command:

*Sec. 2.32 ~**, Sec. 2.33 ~AA0*

Related Topic:

Sec. 3.2 Module Status, Sec. 3.3 Dual Watchdog Operation

2.35 ~AA2

Description: Read Host Watchdog Timeout Interval

Syntax: ~AA2[CHK](cr)

~ delimiter character

AA address of reading module (00 to FF)

2 command for reading host watchdog timeout interval

Response: Valid Command: !AAVV[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

VV timeout interval in HEX format, each count for 0.1 second, 01=0.1 second and FF=25.5 seconds

Example:

Command: ~012

Receive: !01FF

Read address 01 host watchdog timeout interval, return FF, host watchdog timeout interval is 25.5 seconds.

Related Command:

*Sec. 2.32 ~**, Sec. 2.36 ~AA3E VV*

Related Topic:

Sec. 3.2 Module Status, Sec. 3.3 Dual Watchdog Operation

2.36 ~AA3E VV

Description: Set Host Watchdog Timeout Interval

Syntax: ~AA3E VV[CHK](cr)

~ delimiter character
AA address of setting module (00 to FF)
3 command for set host watchdog timeout interval
E 1=Enable/0=Disable host watchdog
VV timeout value, from 01 to FF, each for 0.1 second

Response: Valid Command: !AA[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: ~013164 Receive: !01

Set address 01 enable host watchdog and timeout interval is 64 (10.0 seconds), return success.

Command: ~012 Receive: !0164

Read address 01 host watchdog timeout interval, return timeout interval is 64 (10.0 seconds).

Related Command:

*Sec. 2.32 ~**, Sec. 2.35 ~AA2*

Related Topic:

Sec. 3.2 Module Status, Sec. 3.3 Dual Watchdog Operation

2.37 ~AA4

Description: Read PowerOn Value and Safe Value

Note: The command is for CB-7011/11D/11P/11PD only

Syntax: ~AA4[CHK](cr)

~ delimiter character

AA address of reading module (00 to FF)

4 command for reading PowerOn Value and Safe Value

Response: Valid Command: !AAPPSS[CHK](cr)

Invalid Command: ?AA[CHK](cr)

Syntax error or communication error may get no response.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

PP PowerOn Value, 00=DO0 off, DO1 off, 01=DO0 on, DO1 off, 02=DO0 off, DO1 on, 03=DO0 on, DO1 on

SS Safe Value, data format is same as PP

Example:

Command: ~014

Receive: !010000

Read address 01 Power-On/Safe Value, return Power-On Value is DO0 off, DO1 off, Safe Value is DO0 off, DO1 off.

Related Command:

Sec. 2.38 ~AA5PPSS

Related Topic:

Sec. 3.2 Module Status, Sec. 3.3 Dual Watchdog Operation

2.38 ~AA5PPSS

Description: Set PowerOn Value and Safe Value.

Note: The command is for CB-7011/11D/11P/11PD only.

Syntax: ~AA5PPSS[CHK](cr)

~ delimiter character
AA address of setting module (00 to FF)
5 command for setting PowerOn Value and Safe Value
PP PowerOn Value, 00=DO0 off, DO1 off, 01=DO0 on,
 DO1off, 02=DO0 off, DO1 on, 03=DO0 on, DO1 on
SS Safe Value, data format is same as PP

Response: Valid Command: !AA[CHK](cr)

 Invalid Command: ?AA[CHK](cr)

 Syntax error or communication error may get no re-
 sponse.

! delimiter for valid command

? delimiter for invalid command

AA address of response module(00 to FF)

Example:

Command: ~0150003 Receive: !01

 Set address 01 PowerOn Value is DO0 off, DO1 off, Safe
 Value is DO0 on, DO1 on, return success.

Related Command:

Sec. 2.37 ~AA4

Related Topic:

Sec. 3.2 Module Status, Sec. 3.3 Dual Watchdog Operation

3. Application Note

3.1 INIT* pin Operation

Each CB-7000 module has a build-in EEPROM to store configuration information such as address, type, baud rate and other information. Sometimes, the user may forget the configuration of the module. Therefore, the CB-7000 has a special mode named “INIT mode”, to help the user resolve the problem. The “INIT mode” is setting as Address=00, baud rate = 9600 bps, no checksum.

To enable INIT mode, please follow these steps:

Step 1. Power-down the module.

Step 2. Connect the INIT* pin to the GND pin.

Step 3. Set Power on.

Step 4. Send command \$002(cr) in 9600 bps to read the configuration stored in the module’s EEPROM.

Refer to “CB-7000 Bus Converter User Manual” *Sec. 5.1* and “Getting Started” for more information.

3.2 Module Status

Power-On Reset or **Module Watchdog Reset** will put all outputs to the **Power-On Value**. The module may accept the host’s command to change the output value.

Host Watchdog Timeout will put all digital outputs to the **Safe Value**. The host watchdog timeout flag is set, and the output command will be ignored. The module’s LED will go to flash and user must reset the Module Status via command to restore normal operation.

3.3 Dual Watchdog Operation

Dual Watchdog = Module Watchdog + Host Watchdog

The Module Watchdog is a hardware reset circuit to monitor the module's operating status. While working in harsh or noisy environment, the module may go down by the external noise signal. The circuit may let the module continue to work and never halt.

The Host Watchdog is a software function to monitor the host's operating status. Its purpose is to prevent the network/communication problem or a halted host from causing a dangerous situation. While the timeout occurred, the module will place all outputs to the safe state to prevent from unexpected problem of controlled target.

The CB-7000 module with Dual Watchdog makes the control system more reliable and stable.

3.4 Digital Input and Event Counter

The digital input DI0 can work as event counter. The counter increments when the input changes from high level to low level. The counter has 16 bits and is useful for low speed counting at frequencies lower than 50 Hz.

3.5 Digital Output

When the module powers-on, the host watchdog timeout flag is checked first. If the status is set, the digital outputs (DO0 and DO1) of module are set to the Safe Value. If the flag is clear, the digital outputs are set to the Power-On Value.

If the host watchdog timeout flag is set, the module will

ignore the digital output command @AADO(Data).

3.6 High/Low Alarm

Some analog input modules, such as the CB-7011, are equipped with a high/low alarm function. When the alarm function is enabled, the digital output DO0 is the low alarm indicator, DO1 is the high alarm indicator, and the digital output command for changing digital outputs DO0, DO1 is ignored. The alarm function is to compare the analog input value with given high alarm value and low alarm value. And there are two alarm types as follows:

Momentary alarm: the alarm status is cleared when the analog input is not over the alarm value.

If Analog Input Value $>$ High Alarm, DO1 (High alarm) is on, otherwise DO1 is off.

If Analog Input Value $<$ Low Alarm, DO0 (Low alarm) is on, otherwise DO0 is off.

Latch Alarm: the alarm is cleared only the user send command to clear.

If Analog Input Value $>$ High Alarm, DO1(High alarm) is on, else if Analog Input Value $<$ Low Alarm, DO0(Low alarm) is on.

3.7 Thermocouple Measurement

When two wires composed of dissimilar metal are joined at one end and heated, the open circuit voltage is a function of the junction temperature and the composition of the two metals. All dissimilar metals exhibit this effect. The voltage is called Seebeck voltage". For small changes in temperature the Seebeck voltage is

linearly proportional to temperature.

To measure the Seebeck voltage directly is not available because we must first connect a voltmeter to the thermocouple, and the voltmeter leads themselves create a new thermoelectric (cold) junction. Therefore we need to eliminate the junction thermoelectric to measure the correct Seebeck voltage, and this is called “Cold Junction Compensation”.

For most thermocouples, the Seebeck voltage is 0V while at 0°C. One simple way to cancel the junction voltage is to put the junction into 0°C environment and the junction voltage is 0V. Normally, this is not a good method for most applications. The typical method is to measure the junction temperature with a thermistor, and measure the junction voltage from the junction temperature. Then we can get the Seebeck voltage from measured thermocouple voltage and junction voltage, and we can calculate the temperature from the Seebeck voltage.

For Your Notes

For Your Notes

EC Declaration of Conformity

We, Measurement Computing Corp., declare under sole responsibility that the product:

CB-7011/CB-7011D, Thermocouple Input Modules
CB-7018

Part Number	Description
-------------	-------------

to which this declaration relates, meets the essential requirements, is in conformity with, and CE marking has been applied according to the relevant EC Directives listed below using the relevant section of the following EC standards and other normative documents:

EU EMC Directive 89/336/EEC: Essential requirements relating to electromagnetic compatibility.

EU 55022 Class B: Limits and methods of measurements of radio interference characteristics of information technology equipment.

EN 50082-1: EC generic immunity requirements.

IEC 801-2: Electrostatic discharge requirements for industrial process measurement and control equipment.

IEC 801-3: Radiated electromagnetic field requirements for industrial process measurements and control equipment.

IEC 801-4: Electrically fast transients for industrial process measurement and control equipment.

Carl Haapaoja, Director of Quality Assurance

Measurement Computing Corporation

16 Commerce Blvd.

Middleboro, MA 02346

(508) 946-5100

Fax: (508) 956-9500

E-mail: info@measurementcomputing.com

www.measurementcomputing.com